


NANOCOLOR® Härte 20

Hardness 20 / Dureté 20 / Durezza 20












Test 0-43
REF 985043

Methode / Method / Méthode / Método

- 0431 1–20 °d
- 0432 0,2–3,6 mmol/L
- 0433 1,0–25,0 °e
- 0434 2,0–36,0 °f


540 nm

Min	20–80 %	Max
1	4,8 15,2	20 °d

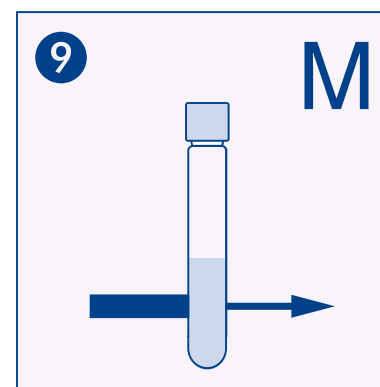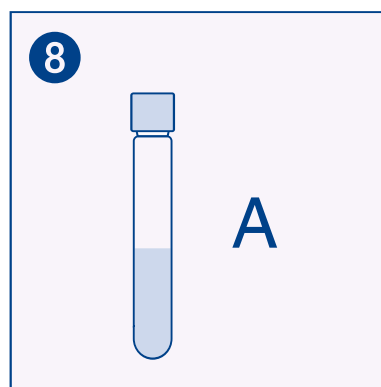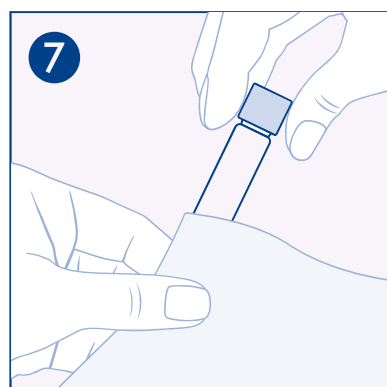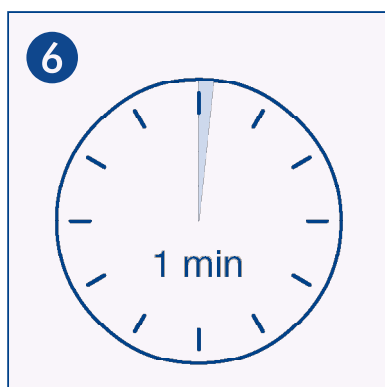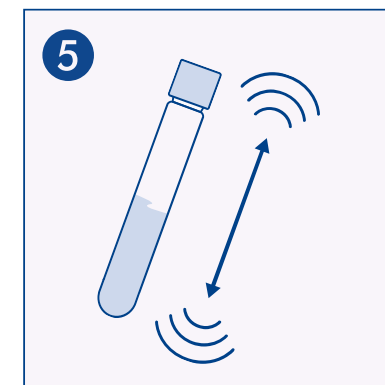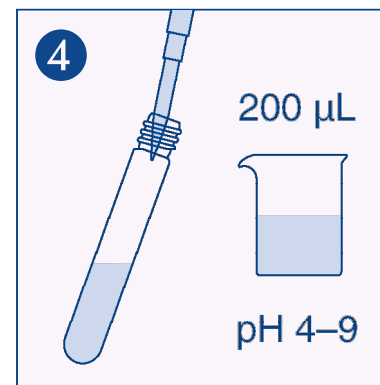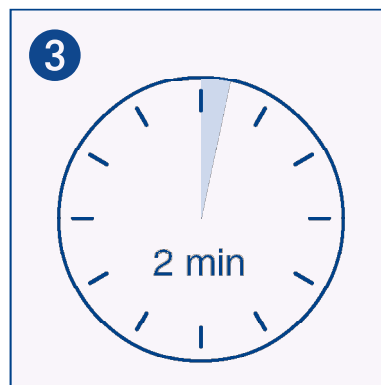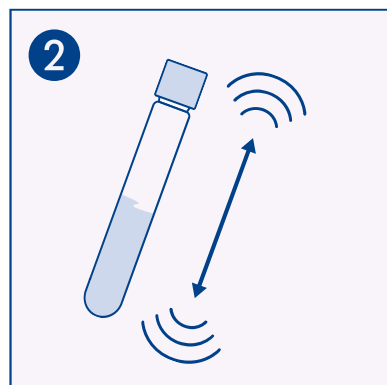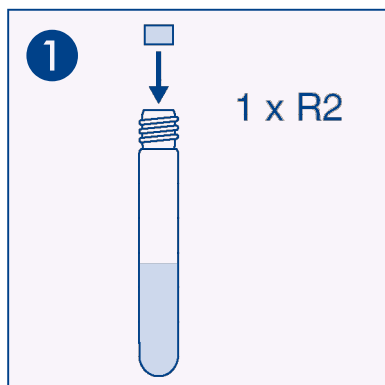

NANOCOLOR® Härte 20

Hardness 20 / Dureté 20 / Durezza 20



Test 0-43
REF 985043

Methode / Method / Méthode / Método

0435 10–100 mg/L Ca

0436 5–50 mg/L Mg

540 nm

Min	20–80 %		Max
10	28	82	100 mg/L Ca
5	14	45	50 mg/L Mg

